



Kent Academic Repository

Marques, M.J., Bradu, A. and Podoleanu, A.G. (2014) *Optical coherence tomography and scanning laser ophthalmoscopy: Approaches to dual-channel retinal tissue imaging*. In: *Frontiers in Optics*, 19 October 2014 - 23 October 2014, Tucson, Arizona, USA.

Downloaded from

<https://kar.kent.ac.uk/49279/> The University of Kent's Academic Repository KAR

The version of record is available from

<https://doi.org/10.1364/FIO.2014.FTu2F.3>

This document version

Pre-print

DOI for this version

Licence for this version

UNSPECIFIED

Additional information

Versions of research works

Versions of Record

If this version is the version of record, it is the same as the published version available on the publisher's web site. Cite as the published version.

Author Accepted Manuscripts

If this document is identified as the Author Accepted Manuscript it is the version after peer review but before type setting, copy editing or publisher branding. Cite as Surname, Initial. (Year) 'Title of article'. To be published in *Title of Journal*, Volume and issue numbers [peer-reviewed accepted version]. Available at: DOI or URL (Accessed: date).

Enquiries

If you have questions about this document contact ResearchSupport@kent.ac.uk. Please include the URL of the record in KAR. If you believe that your, or a third party's rights have been compromised through this document please see our [Take Down policy](https://www.kent.ac.uk/guides/kar-the-kent-academic-repository#policies) (available from <https://www.kent.ac.uk/guides/kar-the-kent-academic-repository#policies>).

Optical Coherence Tomography and Scanning Laser Ophthalmoscopy: approaches to dual-channel retinal tissue imaging

Manuel J. Marques*, Adrian Bradu, and Adrian Gh. Podoleanu

Applied Optics Group, School of Physical Sciences, University of Kent
Canterbury CT2 7NH, United Kingdom

*mjmm2@kent.ac.uk

Abstract: We report a Talbot bands-based optical coherence tomography (OCT) system capable of producing longitudinal B-scan OCT images and *en-face* scanning laser ophthalmoscopy (SLO) images of the human retina *in-vivo*, with various degrees of simultaneity.

© 2014 Optical Society of America

OCIS codes: (110.4190) Imaging systems: Multiple imaging; (110.4500) Imaging systems: Optical coherence tomography; (170.4460) Medical optics and biotechnology: Ophthalmic optics and devices;

Due to a higher sensitivity and speed than their time domain (TD) counterpart, spectral domain (SD) methods dominate the OCT technology of eye imaging [1]. The SD-OCT methods produce fast A-scans, which are used to create real time cross-section (B-scan) images.

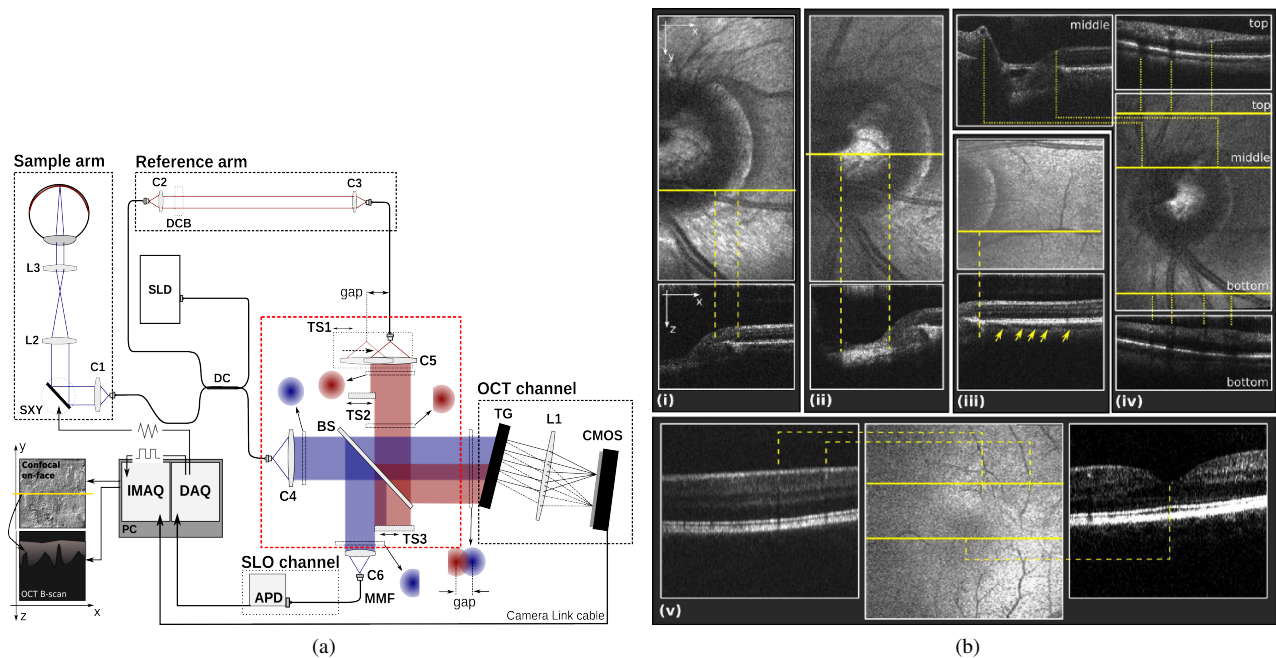


Fig. 1: (a) Schematic representation of the set-up devised, and (b) some of the results obtained with it: images of the retina of a volunteer taken from the two channels, yielding an *en-face* SLO image (top) and a B-scan OCT image (bottom), with a correspondence of features between the two being emphasized.

For several reasons, an *en-face* image is also required when imaging the retina in the human eye. These reasons may include the guidance of the OCT examination, or even the correction of motion artifacts created by imaging *in-vivo*

tissues with a low degree of fixation. SD-OCT methods allow the creation of such images, however when scanning over the two orthogonal directions it is inevitable to obtain a full volumetric image, which will have to be post-processed, the image being then displayed static to the user.

Several other techniques are available to generate an *en-face* image without resorting to a SD-OCT based method, which show the interest for presenting such images alongside the SD-OCT investigation delivering B-scans, with a good pixel-to-pixel correspondence between the two frames.

Our method [2] involves a SD-OCT system (schematically described in Fig. 1a) whose spectrometer system has been modified to take advantage of Talbot bands [3]: the degree of overlapping between the two beams returning from the interferometer on their way to the diffractive medium can be controlled and employed to shift the SD-OCT sensitivity profile maximum away from the interferometer's alignment point. This implementation involves a beam-splitter *BS* to couple the two beams, and by placing a specially-devised filter over the beam path that would not otherwise be used, one is capable of spatially separate the two components, therefore isolating the optical power returning from the sample and directing it to a highly-sensitive detector, forming a confocal image which is acquired in tandem and with the same interface optics as the OCT image. Given that the system in question is used to image human retinal tissue, the confocal channel will yield images similar to the ones produced by a scanning laser ophthalmoscope (SLO). The two frames are then acquired: an *en-face* SLO image and a depth profile (B-scan OCT), whose lateral position can be controlled by means of a cursor overlaid on the SLO frame.

With adequate acquisition and control systems in place, it is then possible to acquire these two frames with varying degrees of simultaneity and pixel-to-pixel correspondence. The constraints present are purely related to the speeds of acquisition and scanning provided by current technology: the fastest CMOS camera in near-IR available is capable of performing up to 312,500 spectral reads per second [4] and current galvo-scanner technology (preferred over faster scanning techniques, such as resonant scanners, to implement some of the operating modes described in [2]) cannot exceed a scanning rate of 1 kHz. One is capable of true simultaneity in terms of image acquisition *and* refresh if the transversal range is sacrificed; conversely, if larger transversal ranges are desired the two channels will have to be read sequentially.

Figure 1b features some of the results obtained with the system described. In all pairs of frames the retina from the same volunteer is being imaged in different regions, with varying lateral sizes (from 2.6 to 5 mm). The Talbot bands allow for an improvement of the OCT channel sensitivity at larger depths (measured up to 6 dB), thus reducing the occurrence of mirror terms by reducing the need to place the sample very close to the alignment point of the interferometer.

With this method it is then possible to achieve simultaneous imaging of the two channels within the hardware-related constraints. This will allow the clinician to have more information when performing an investigative analysis, as one can guide the OCT-based depth profiling using a "bird's eye" view provided by the SLO imagery.

Acknowledgements

M. J. Marques acknowledges the support of the University of Kent through his University Scholarship. A. Bradu and A. Gh. Podoleanu acknowledge the support of the European Research Council (ERC) (<http://erc.europa.eu>) CO-GATIMABIO 249889. A. Podoleanu is also supported by the NIHR Biomedical Research Centre at Moorfields Eye Hospital NHS Foundation Trust and UCL Institute of Ophthalmology.

References

1. M. Wojtkowski, R. Leitgeb, A. Kowalczyk, T. Bajraszewski, and A. F. Fercher, "In vivo human retinal imaging by Fourier domain optical coherence tomography." *J. Biomed. Opt.* **7**, 457–63 (2002).
2. M. J. Marques, A. Bradu, and A. G. Podoleanu, "Towards simultaneous Talbot bands based optical coherence tomography and scanning laser ophthalmoscopy imaging," *Biomed. Opt. Express* **5**, 1428–1444 (2014).
3. A. Gh. Podoleanu, "Unique interpretation of Talbot Bands and Fourier domain white light interferometry," *Opt. Express* **15**, 9867–9876 (2007).
4. B. Potsaid, I. Gorczynska, V. J. Srinivasan, Y. Chen, J. Jiang, A. Cable, and J. G. Fujimoto, "Ultrahigh speed spectral/Fourier domain OCT ophthalmic imaging at 70,000 to 312,500 axial scans per second," *Opt. Express* **16**, 15149–15169 (2008).